

T C A T C G T A T C C A T C C C T A T C C A T C C C T
C A T C C C T A T C G C T T C C A T C T G C T T C A
T C T T C A T C C G T A T C T G C T T C C A T C T G C T
C A T T T C A T C C G T A T C C A T C T G C T
C T T C C A T C C C T A T C G C
C A T C C A T C C C T A T C T G C T T C C A T C T G C T



BIOTECON

Diagnostics

Product List

- Kits & Reagents




Bacterial Pathogens
Viral Pathogens
Beverage Spoilage Organisms
Yeast and Mold
GMOs
Allergens
Animal Identification
Veterinary
Environmental
Pharma
DNA/RNA Extraction
Additional Products

Valid from November 2017

EuroClone®
serving science through innovation

EUROCLONE SpA - Via Figino, 20/2220016 Pero (MI) Italy - Tel. +39 02 38195.1 - Fax +39 02 33913713
info@euroclone.it - www.euroclone.it

Azienda con Sistema di Gestione della Qualità certificato EN ISO 9001 - ENISO 13485 e Gestione Ambientale certificato EN ISO 14001

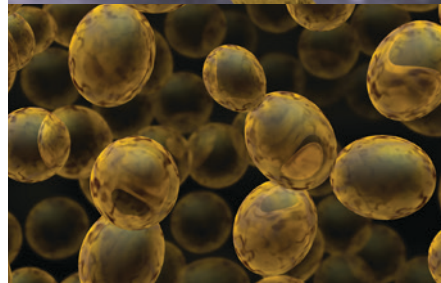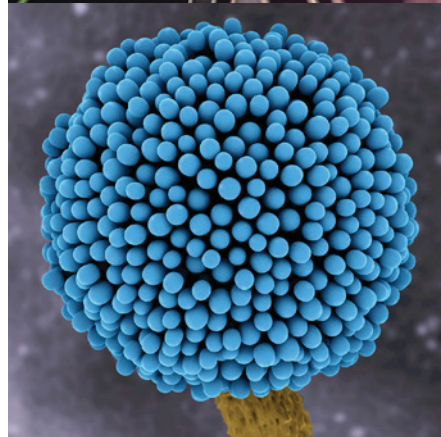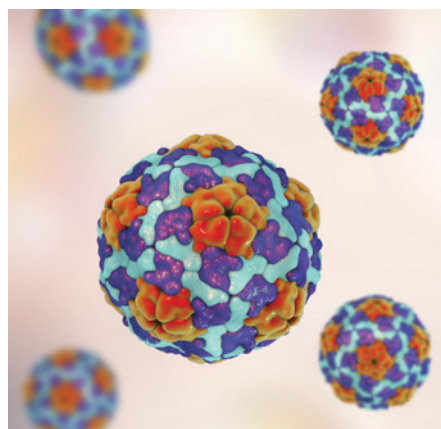

| order no. | real-time PCR Kits | reactions | applicable to | | | |
|----------------------------|---------------------------------------------------------------------------------------|-----------|---------------|--------|--------------------------------|----------------------|
| | | | LC 2.0 | LC 480 | LC 96, PikoReal 24, and other* | Mx3005p, and other** |
| Bacterial Pathogens | | | | | | |
| <i>Salmonella</i> | | | | | | |
| R 602 27-1 | foodproof® <i>Salmonella</i> Detection LyoKit - LP (AOAC-RI) | 96 | - | + | + | - |
| R 602 27-2 | foodproof® <i>Salmonella</i> Detection LyoKit - RP (AOAC-RI) | 96 | - | - | - | + |
| R 602 27-1 L | foodproof® <i>Salmonella</i> Detection LyoKit - LP (AOAC-RI) | 480 | - | + | + | - |
| R 602 27-2 L | foodproof® <i>Salmonella</i> Detection LyoKit - RP (AOAC-RI) | 480 | - | - | - | + |
| R 302 27 | foodproof® <i>Salmonella</i> Detection Kit (AOAC-RI + MicroVal + NordVal + DAFF) | 96 | - | + | + | + |
| R 302 27 L | foodproof® <i>Salmonella</i> Detection Kit (AOAC-RI + MicroVal + NordVal + DAFF) | 480 | - | + | + | + |
| R 310 27 | foodproof® <i>Salmonella</i> Detection Kit (AOAC-RI + MicroVal + NordVal + DAFF) | 96 | + | + | - | - |
| R 602 34-1 | foodproof® <i>Salmonella</i> Enteritidis & Typhimurium Detection LyoKit - LP | 96 | - | + | + | - |
| R 602 34-2 | foodproof® <i>Salmonella</i> Enteritidis & Typhimurium Detection LyoKit - RP | 96 | - | - | - | + |
| <i>Listeria</i> | | | | | | |
| R 602 20-1 | foodproof® <i>Listeria</i> Genus Detection LyoKit - LP | 96 | - | + | + | - |
| R 602 20-2 | foodproof® <i>Listeria</i> Genus Detection LyoKit - RP | 96 | - | - | - | + |
| R 302 20 | foodproof® <i>Listeria</i> Genus Detection Kit | 96 | - | + | + | + |
| R 300 20 | foodproof® <i>Listeria</i> Genus Detection Kit | 96 | + | + | - | - |
| R 602 23-1 | foodproof® <i>Listeria monocytogenes</i> Detection LyoKit - LP | 96 | - | + | + | - |
| R 602 23-2 | foodproof® <i>Listeria monocytogenes</i> Detection LyoKit - RP | 96 | - | - | - | + |
| R 302 23 | foodproof® <i>Listeria monocytogenes</i> Detection Kit (AOAC-RI + NordVal) | 96 | - | + | + | + |
| R 300 23 | foodproof® <i>Listeria monocytogenes</i> Detection Kit (AOAC-RI + NordVal) | 96 | + | + | - | - |
| <i>Escherichia coli</i> | | | | | | |
| R 302 10 | foodproof® <i>E. coli</i> O157 Detection Kit (AOAC-RI + NordVal) | 96 | - | + | + | + |
| R 300 10 | foodproof® <i>E. coli</i> O157 Detection Kit (AOAC-RI + NordVal) | 96 | + | - | - | - |
| R 300 09 | foodproof® <i>E. coli</i> and <i>Shigella</i> Detection Kit | 96 | + | + | - | - |
| F 602 09-1 | foodproof® <i>E. coli</i> and <i>Shigella</i> LyoKit - LP | 96 | - | + | + | - |
| F 602 09-2 | foodproof® <i>E. coli</i> and <i>Shigella</i> LyoKit - RP | 96 | - | - | - | + |
| R 602 11-1 | foodproof® STEC Screening LyoKit - LP | 96 | - | + | + | - |
| R 602 11-2 | foodproof® STEC Screening LyoKit - RP | 96 | - | - | - | + |
| R 602 12-1 | foodproof® STEC Identification LyoKit - LP | 48 | - | + | + | - |
| R 602 12-2 | foodproof® STEC Identification LyoKit - RP | 48 | - | - | - | + |
| <i>Campylobacter</i> | | | | | | |
| R 302 05 | foodproof® <i>Campylobacter</i> Quantification Kit | 96 | - | + | + | + |
| R 310 05 | foodproof® <i>Campylobacter</i> Detection Kit | 96 | + | + | - | - |
| <i>Cronobacter</i> | | | | | | |
| R 302 15.1 | foodproof® <i>Enterobacteriaceae</i> plus <i>Cronobacter</i> Detection Kit (MicroVal) | 96 | - | + | + | + |
| R 310 15.1 | foodproof® <i>Enterobacteriaceae</i> plus <i>Cronobacter</i> Detection Kit (MicroVal) | 96 | + | + | - | - |
| R 310 15.1 L | foodproof® <i>Enterobacteriaceae</i> plus <i>Cronobacter</i> Detection Kit (MicroVal) | 480 | + | + | - | - |
| R 602 13 -1 | foodproof® <i>Cronobacter</i> Detection LyoKit - LP | 96 | - | + | + | - |
| R 602 13 -2 | foodproof® <i>Cronobacter</i> Detection LyoKit - RP | 96 | - | - | - | + |

* AriaMX, ABI 7500 Fast, Biorad CFX96 and other 5'Nuclease technology-based real-time PCR cyclers for low profile (please request)

** ABI 7500 and other 5'Nuclease technology-based real-time PCR cyclers for regular profile (please request)

Note: RDK = Pre-Launch Version, LP = Low Profile, RP = Regular Profile, DP = Different Profile

foodproof®, microproof® and vetproof® are registered trademarks of BIOTECON Diagnostics. The above mentioned real-time PCR instruments are registered trademarks of their respective holders.

| order no. | real-time PCR Kits | reactions | applicable to | | | |
|------------------------------------|---------------------------------------------------------------------------------------|-----------|---------------|--------|--------------------------------|----------------------|
| | | | LC 2.0 | LC 480 | LC 96, PikoReal 24, and other* | Mx3005p, and other** |
| Vibrio | | | | | | |
| R 602 44-1 | foodproof® <i>Vibrio</i> Detection LyoKit - LP | 96 | - | + | + | - |
| R 602 44-2 | foodproof® <i>Vibrio</i> Detection LyoKit - RP | 96 | - | - | - | + |
| Clostridium | | | | | | |
| R 602 40-1 | foodproof® <i>Clostridium botulinum</i> Detection LyoKit - LP | 96 | - | + | + | - |
| R 602 40-2 | foodproof® <i>Clostridium botulinum</i> Detection LyoKit - RP | 96 | - | - | - | + |
| F 302 41 | foodproof® <i>Clostridium</i> Control Detection Kit | 64 | - | + | + | + |
| Z 700 08 | foodproof® SL <i>Clostridium perfringens</i> Detection Kit | 50 | - | + | + | + |
| Other Pathogens | | | | | | |
| R 302 04 | foodproof® <i>Brucella</i> Detection Kit | 96 | - | + | + | + |
| F 302 49 | foodproof® <i>Yersinia enterocolitica</i> Detection Kit | 96 | - | + | + | + |
| F 302 53 | foodproof® <i>Yersinia enterocolitica</i> and <i>pseudotuberculosis</i> Detection Kit | 48 | - | + | + | + |
| Z 700 05 | foodproof® SL <i>Staphylococcus aureus</i> Detection Kit | 50 | - | + | + | + |
| Z 700 06 | foodproof® SL <i>Bacillus cereus</i> Detection Kit | 50 | - | + | + | + |
| Viral Pathogens | | | | | | |
| R 302 37 | foodproof® Hepatitis A Virus Detection Kit | 64 | - | + | + | + |
| R 302 38.1 | foodproof® Norovirus Detection Kit (GI, GII) | 64 | - | + | + | + |
| R 302 50 | foodproof® Norovirus (GI, GII) plus Hepatitis A Virus Detection Kit | 64 | - | + | + | + |
| Beverage Spoilage Organisms | | | | | | |
| R 602 02-1 | foodproof® Beer Screening LyoKit - LP | 96 | - | + | + | - |
| R 602 02-2 | foodproof® Beer Screening LyoKit - RP | 96 | - | - | - | + |
| R 602 02-3 | foodproof® Beer Screening LyoKit - DP | 96 | MyGoPro | | | |
| R 310 02 | foodproof® Beer Screening Kit | 96 | + | + | - | - |
| R 302 28 | foodproof® <i>Alicyclobacillus</i> Detection Kit | 96 | - | + | + | + |
| R 302 08 | foodproof® <i>Dekkera</i> Quantification Kit | 96 | - | + | + | + |
| R 300 26 | foodproof® <i>Saccharomyces cerevisiae</i> var. <i>diastaticus</i> Detection Kit | 96 | + | + | - | - |
| RDK 100 37-1 | foodproof® Spoilage Yeast Detection 1 LyoKit - LP | 48 | - | + | + | - |
| RDK 100 37-2 | foodproof® Spoilage Yeast Detection 1 LyoKit - RP | 48 | - | - | - | + |
| RDK 100 37-3 | foodproof® Spoilage Yeast Detection 1 LyoKit - DP | 48 | MyGoPro | | | |
| RDK 100 38-1 | foodproof® Spoilage Yeast Detection 2 LyoKit - LP | 48 | - | + | + | - |
| RDK 100 38-2 | foodproof® Spoilage Yeast Detection 2 LyoKit - RP | 48 | - | - | - | + |
| RDK 100 38-3 | foodproof® Spoilage Yeast Detection 2 LyoKit - DP | 48 | MyGoPro | | | |
| Yeast & Mold | | | | | | |
| R 602 42-1 | foodproof® Yeast and Mold Quantification LyoKit - LP | 96 | - | + | + | - |
| R 602 42-2 | foodproof® Yeast and Mold Quantification LyoKit - RP | 96 | - | - | - | + |
| R 602 42-3 | foodproof® Yeast and Mold Quantification LyoKit - DP | 96 | MyGoPro | | | |

* AriaMX, ABI 7500 Fast, Biorad CFX96 and other 5'Nuclease technology-based real-time PCR cyclers for low profile (please request)

** ABI 7500 and other 5'Nuclease technology-based real-time PCR cyclers for regular profile (please request)

Note: RDK = Pre-Launch Version, LP = Low Profile, RP = Regular Profile, DP = Different Profile

foodproof®, microproof® and vetproof® are registered trademarks of BIOTECON Diagnostics. The above mentioned real-time PCR instruments are registered trademarks of their respective holders.

Product List - Kits & Reagents

| order no. | real-time PCR Kits | reactions | applicable to | | | |
|-------------------------------------|---------------------------------------------------------------------------------------------------|-----------|---------------|--------|-------------------------------|----------------------|
| | | | LC 2.0 | LC 480 | LC 96, PikoReal24, and other* | Mx3005p, and other** |
| GMOs | | | | | | |
| GMO Screening | | | | | | |
| R 602 17-1 | foodproof® GMO Screening 1 LyoKit - LP (35S, NOS, FMV) | 96 | - | + | + | - |
| R 602 17-2 | foodproof® GMO Screening 1 LyoKit - RP (35S, NOS, FMV) | 96 | - | - | - | + |
| R 602 18-1 | foodproof® GMO Screening 2 LyoKit - LP (bar, P-35S-pat, CTP2-CP4-EPSPS, P-NOS-nptII, P-35S-nptII) | 96 | - | + | + | - |
| R 602 18-2 | foodproof® GMO Screening 2 LyoKit - RP (bar, P-35S-pat, CTP2-CP4-EPSPS, P-NOS-nptII, P-35S-nptII) | 96 | - | - | - | + |
| R 302 17 | foodproof® GMO Screening Kit (35S, NOS, bar, FMV), plant assay included | 2x 64 | - | + | + | + |
| R 300 17 | foodproof® GMO Screening Kit (35S, NOS), plant assay included | 2x 64 | + | + | - | - |
| R 602 21-1 | foodproof® Plant Detection LyoKit - LP | 96 | - | + | + | - |
| R 602 21-2 | foodproof® Plant Detection LyoKit - RP | 96 | - | - | - | + |
| GMO Identification | | | | | | |
| Z 722 01 | foodproof® SL GMO A2704-12 Soya Detection Kit | 50 | - | + | + | + |
| Z 722 02 | foodproof® SL GMO GTS40-3-2 Soya Detection Kit | 50 | - | + | + | + |
| Z 720 01 | foodproof® SL GMO Bt11 Maize Detection Kit | 50 | - | + | + | + |
| Z 720 11 | foodproof® SL GMO DAS59112-7 Maize Detection Kit | 50 | - | + | + | + |
| Z 720 02 | foodproof® SL GMO GA21 Maize Detection Kit | 50 | - | + | + | + |
| Z 720 05 | foodproof® SL GMO MIR162 Maize Detection Kit | 50 | - | + | + | + |
| Z 720 06 | foodproof® SL GMO MIR604 Maize Detection Kit | 50 | - | + | + | + |
| Z 720 03 | foodproof® SL GMO MON810 Maize Detection Kit | 50 | - | + | + | + |
| Z 720 12 | foodproof® SL GMO MON863 Maize Detection Kit | 50 | - | + | + | + |
| Z 720 07 | foodproof® SL GMO MON88017 Maize Detection Kit | 50 | - | + | + | + |
| Z 720 08 | foodproof® SL GMO MON89034 Maize Detection Kit | 50 | - | + | + | + |
| Z 720 09 | foodproof® SL GMO NK603 Maize Detection Kit | 50 | - | + | + | + |
| Z 720 04 | foodproof® SL GMO T25 Maize Detection Kit | 50 | - | + | + | + |
| Z 720 10 | foodproof® SL GMO TC1507 Maize Detection Kit | 50 | - | + | + | + |
| GMO Multiplex Identification | | | | | | |
| R 602 24 | foodproof® GMO Soya Identification 1 LyoKit (DAS-44406-6, MON87701, MON87708, MON87769) | 96 | - | + | + | + |
| R 602 25 | foodproof® GMO Soya Identification 2 LyoKit (BPS-CV127-9, DP-305423-1, DAS-68416-4, DAS-81419-2) | 96 | - | + | + | + |
| F 602 46 | foodproof® GMO Maize Identification 1 LyoKit (DAS-40278-9, LY038, VCO-01981-5) | 96 | - | + | + | + |
| Z 725 01 | foodproof® SL GMO Maize Multiplex Detection Kit (GA21, MIR604) | 50 | - | + | + | + |
| Z 725 02 | foodproof® SL GMO Maize Multiplex Detection Kit (MON89034, CBH351, Bt176) | 50 | - | + | + | + |
| Z 725 03 | foodproof® SL GMO Maize Multiplex Detection Kit (MON88017, NK603, MIR162) | 50 | - | + | + | + |
| Z 725 06 | foodproof® SL GMO Maize Multiplex Detection Kit (Bt11, TC1507) | 50 | - | + | + | + |
| Z 725 07 | foodproof® SL GMO Maize Multiplex Detection Kit (T25, MON810, MON863) | 50 | - | + | + | + |
| GMO Quantification | | | | | | |
| R 302 29 | foodproof® GMO 35S Maize Quantification Kit | 2x 64 | - | + | + | + |
| R 302 16 | foodproof® GMO Bt176 Maize Quantification Kit | 2x 64 | + | + | + | + |
| R 302 19 | foodproof® GMO RR Soya Quantification Kit | 2x 64 | - | + | + | + |
| R 302 35 | foodproof® GMO RR 2 Yield Soya Quantification Kit | 2x 64 | - | + | + | + |

* AriaMX, ABI 7500 Fast, Biorad CFX96 and other 5'Nuclease technology-based real-time PCR cyclers for low profile (please request)

** ABI 7500 and other 5'Nuclease technology-based real-time PCR cyclers for regular profile (please request)

Note: RDK = Pre-Launch Version, LP = Low Profile, RP = Regular Profile, DP = Different Profile

foodproof®, microproof® and vetproof® are registered trademarks of BIOTECON Diagnostics. The above mentioned real-time PCR instruments are registered trademarks of their respective holders.

Product List - Kits & Reagents

| order no. | real-time PCR Kits | reactions | applicable to | | | |
|------------------------------|-----------------------------------------------------------------------------------------------------|-----------|--------------------------------------|--------|--------------------------------|----------------------|
| | | | LC 2.0 | LC 480 | LC 96, PikoReal 24, and other* | Mx3005p, and other** |
| Allergens | | | | | | |
| R 302 60 | foodproof® Celery Detection Kit | 64 | - | + | + | + |
| R 302 61 | foodproof® Soya Detection Kit | 64 | - | + | + | + |
| R 302 62 | foodproof® Hazelnut Detection Kit | 64 | - | + | + | + |
| R 302 63 | foodproof® Peanut Detection Kit | 64 | - | + | + | + |
| R 302 64 | foodproof® Gluten Detection Kit | 64 | - | + | + | + |
| Animal Identification | | | | | | |
| R 602 43-1 | foodproof® Porcine Detection LyoKit - LP | 96 | - | + | + | - |
| R 602 43-2 | foodproof® Porcine Detection LyoKit - RP | 96 | - | - | - | + |
| RDK 100 39-1 | foodproof® Animal Detection 1 LyoKit (Porcine, Bovine, Equine) - LP | 96 | - | + | + | - |
| RDK 100 39-2 | foodproof® Animal Detection 1 LyoKit (Porcine, Bovine, Equine) - RP | 96 | - | - | - | + |
| F 602 54 | foodproof® Water Buffalo Detection LyoKit | 96 | - | - | - | + |
| Z 730 02 | foodproof® SL Bovine Species Detection Kit | 50 | - | + | + | + |
| Z 730 03 | foodproof® SL Sheep Species Detection Kit | 50 | - | + | + | + |
| Z 730 04 | foodproof® SL Horse Species Detection Kit | 50 | - | + | + | + |
| Z 730 05 | foodproof® SL Chicken Species Detection Kit | 50 | - | + | + | + |
| Z 730 06 | foodproof® SL Goat Species Detection Kit | 50 | - | + | + | + |
| Z 730 07 | foodproof® SL Duck Species Detection Kit | 50 | - | + | + | + |
| Z 730 08 | foodproof® SL Shrimp and Crab Species Detection Kit | 50 | - | + | + | + |
| Veterinary | | | | | | |
| V 900 01 | vetproof® SE Vaccine Detection 1 Kit*** | 48 | - | + | + | - |
| V 900 27 | vetproof® Salmonella Detection Kit*** | 96 | - | + | + | - |
| V 740 01 | vetproof® SL Mycoplasma Multiplex Detection Kit (<i>M. gallisepticum</i> , <i>M. synoviae</i>)*** | 100 | - | + | + | + |
| Environmental | | | | | | |
| R 602 45-1 | microproof® Legionella Quantification LyoKit - LP | 96 | - | + | + | - |
| R 602 45-2 | microproof® Legionella Quantification LyoKit - RP | 96 | - | - | - | + |
| Pharma | | | | | | |
| R 300 31 | microproof® Hygiene Screening System | 96 | + | + | - | - |
| R 300 32 | microproof® Streptococcus pneumoniae Detection Kit | 96 | + | + | - | - |
| Additional Products | | | | | | |
| Color Compensation Kits | | runs | | | | |
| A 500 08 | Color Compensation Set 1 | 5 | - | + | - | - |
| A 500 10 | Color Compensation Set 3 | 5 | - | + | - | - |
| A 500 11 | Color Compensation Set 4 | 5 | + | - | - | - |
| A 500 15 | Color Compensation Set 5 | 5 | - | + | - | - |
| Other | | | applicable to | | | |
| A 500 01 | Enzyme Mix (Taq Polymerase / UNG) | | microproof® Hygiene Screening System | | | |
| A 500 13 | Allergen RM 800 Reference Material | | foodproof® Allergen Detection Kits | | | |

* AriaMX, ABI 7500 Fast, Biorad CFX96 and other 5'Nuclease technology-based real-time PCR cyclers for low profile (please request)

** ABI 7500 and other 5'Nuclease technology-based real-time PCR cyclers for regular profile (please request)

*** Regulatory requirements vary by country; products may not be available in your geographic area

Note: RDK = Pre-Launch Version, LP = Low Profile, RP = Regular Profile, DP = Different Profile

foodproof®, microproof® and vetproof® are registered trademarks of BIOTECON Diagnostics. The above mentioned real-time PCR instruments are registered trademarks of their respective holders.

| order no. | DNA/RNA Extraction Kits | reactions | applicable to |
|-----------------|----------------------------------------------|-----------|---------------------------------------------------------------------------------------------|
| StarPrep | | | |
| S 400 07 | foodproof® StarPrep One Kit (AOAC, MicroVal) | 100 | Enterobacteriaceae, Salmonella, Cronobacter, E. coli, Shigella |
| S 400 07 L | foodproof® StarPrep One Kit (AOAC, MicroVal) | 500 | Enterobacteriaceae, Salmonella, Cronobacter, E. coli, Shigella |
| S 400 08 | foodproof® StarPrep Two Kit | n.a.* | Listeria, Campylobacter, Beer Spoilage Bacteria, Alicyclobacillus, Legionella, Yeast & Mold |
| S 400 17 L | foodproof® StarPrep Two 8-Strip Kit | 480 | Listeria |
| S 400 18 | foodproof® StarPrep Three Kit | n.a.* | Beer Spoilage Bacteria, Vibrio, STEC, Animal Detection 1, SE Vaccine Detection |
| S 400 09 | foodproof® StarPrep Four Kit | 96 | Dekkera |

| | | | |
|------------------|---------------------------------------------|----|--------------------------------------------|
| ShortPrep | | | |
| S 400 01 | foodproof® ShortPrep I Kit (AOAC, NordVal) | 96 | Salmonella |
| S 400 02 | foodproof® ShortPrep II Kit (AOAC, NordVal) | 96 | Listeria, Campylobacter, E. coli, Shigella |

| | | | |
|---------------------------|---------------------------------------|-----|----------------------------------------------------------------|
| Sample Preparation | | | |
| S 400 04 | foodproof® Sample Preparation Kit I | 100 | Enterobacteriaceae, Salmonella, Cronobacter, E. coli, Shigella |
| S 400 05 | foodproof® Sample Preparation Kit II | 100 | Listeria, Campylobacter, Alicyclobacillus |
| S 400 06.1 | foodproof® Sample Preparation Kit III | 50 | GMOs, Allergens and Animal ID |
| S 400 16 | foodproof® Sample Preparation Kit IV | 50 | Viruses |

| | | | |
|-----------------------------|--------------------------------------------------------|-----|---------------------------------------------|
| Magnetic Preparation | | | |
| S 400 11 | foodproof® Magnetic Preparation Kit I (AOAC, MicroVal) | 96 | Salmonella, Cronobacter, E. coli, Shigella |
| S 400 11 L | foodproof® Magnetic Preparation Kit I (AOAC, MicroVal) | 480 | Salmonella, Cronobacter, E. coli, Shigella |
| S 400 12 L | foodproof® Magnetic Preparation Kit II | 480 | Listeria |
| S 400 13 L | foodproof® Magnetic Preparation Kit III | 480 | GMOs, Allergens and Animal ID |
| S 400 15 L | foodproof® Magnetic Preparation Kit IV | 480 | Enterobacteriaceae, Salmonella, Cronobacter |
| S 400 19 L | foodproof® Magnetic Preparation Kit V | 480 | Salmonella in PPS samples |
| RDK 100 43 | foodproof® Magnetic Preparation Kit VI | 480 | Veterinary Viruses |

| | | | |
|----------------------------|-------------------------------|--------------------------------------------------------------------------------------------|--|
| Additional Products | | | |
| Reagents | | applicable to | |
| A 500 02 S | Reagent D, 15 ml (MicroVal) | Vibrio | |
| A 500 02 | Reagent D, 30 ml (MicroVal) | Enterobacteriaceae, Cronobacter, Legionella, Yeast & Mold, Spoilage Yeast | |
| A 500 02 L | Reagent D, 150 ml (MicroVal) | Enterobacteriaceae, Cronobacter | |
| A 500 12 | Reagent P | Animal ID, foodproof® Magnetic Preparation Kit I, virus concentration protocol for seafood | |
| A 500 14 | Resuspension Reagent | foodproof® Star Prep Two Kit | |
| A 500 18 | Rinse Buffer | Legionella | |
| Other | | applicable to | |
| S 400 10 | Suspension Buffer | microproof® Hygiene Screening System | |
| Z 800 01 | foodproof® Listeria StarBroth | Listeria monocytogenes, Listeria Genus | |

* Number of isolations depending on parameter
 foodproof® and microproof® are registered trademarks of BIOTECON Diagnostics.